

ORAL PRESENTATION

Open Access

Real-time MR-guided transarterial aortic valve implantation (tavi): in vivo evaluation in swine

Harald H Quick^{1*}, Philipp Kahlert², Holger Eggebrecht², Gernot M Kaiser³, Nina Parohl⁴, Juliane Albert⁴, Lena Schäfer⁴, Ian McDougall⁵, Raimund Erbel², Mark E Ladd⁴

From 2011 SCMR/Euro CMR Joint Scientific Sessions
Nice, France. 3-6 February 2011

Objective

Transcatheter, transarterial aortic valve implantation (TAVI) is rapidly emerging as a promising new treatment option for patients with severe symptomatic aortic valve stenosis who are considered at high or prohibitive surgical risk. Envisioning real-time MR guidance of the TAVI procedure, the objective of this study was the systematical *in vitro* evaluation of the MR imaging characteristics of a currently commercially available TAVI prosthesis and its delivery device and subsequent modification of the delivery device towards MR-compatibility. Featuring the modified MR compatible stent valve delivery device, real-time MR guided TAVI has been performed *in vivo* in eight swine.

Methods

The self-expandable Medtronic CoreValve[®] aortic bioprosthesis (Medtronic, Minneapolis, USA) is composed of a nitinol stent frame with an integrated trileaflet porcine pericardial tissue valve and is either implanted via the femoral or subclavian artery. Its delivery catheter has a 12Fr shaft with 18Fr distal end comprising the crimped prosthesis which can be released stepwise. The original catheter shaft revealed ferromagnetic attraction thus potentially compromising MR imaging and safety. The delivery device consequently was re-designed obviating any metal braiding resulting in full MR compatibility of the delivery device. MR-guided TAVI was performed on 8 farm pigs (75-85 kg) via transfemoral (2/8) and via subclavian (6/8) access on a 1.5 T MRI system (Avanto, Siemens, Germany) equipped with an interventional in-room monitor. Catheter placement and

stent release was performed under real-time MR-guidance with a rt-TrueFISP sequence providing 5 fps.

Results

The nitinol-based self-expandable stent-valve was excellently visualized with delineation even of small details. The commercial delivery catheter shaft of this device revealed strong ferromagnetic artifacts, thus also raising concerns regarding RF-related device heating and ferromagnetic attraction. Replacement of the commercial delivery device by the re-designed delivery device resulted in artifact elimination and excellent real-time visualization of catheter movement and valve deployment. MR-guided TAVI was successful in 6/8 swine (Figure 1). Post-interventional therapeutic success could be confirmed using ECG-triggered cine-TrueFISP sequences and flow-sensitive phase contrast sequences. Final stent valve position was confirmed by *ex vivo* histology.

Conclusions

The self-expandable CoreValve aortic stent-valve is potentially suited for real-time MRI-guided placement after suggested design modifications of the delivery-system. MR imaging in this interventional setup provided excellent pre-interventional anatomic and functional evaluation of the native aortic valve, precise real-time instrument guidance allowing accurate placement of the stent-valve within the native aortic annulus, and finally detailed post-interventional evaluation of therapeutic success.

¹Institute of Medical Physics, University of Erlangen, Erlangen, Germany
Full list of author information is available at the end of the article

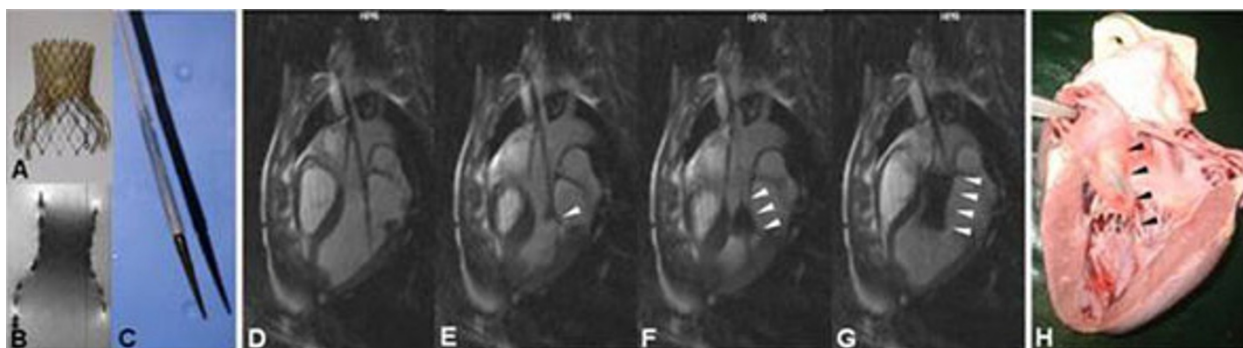


Figure 1 Nitinol CoreValve (A) featuring an aortic valve formed from porcine pericardial tissue, MR image (B); modified MR compatible delivery catheter (C). (D-G) Real-time TrueFISP images of MR-guided CoreValve deployment in vivo. Arrowheads in (E-G) show successive stent release and final stent position in histologic correlation (H).

Author details

¹Institute of Medical Physics, University of Erlangen, Erlangen, Germany.

²Department of Cardiology, University Hospital Essen, Essen, Germany.

³Department of Transplantation Surgery, University Hospital Essen, Essen, Germany.

⁴Institute of Diagnostic and Interventional Radiology, University Hospital Essen, Essen, Germany.

⁵Evasec Medical Systems, Vancouver, BC, Canada.

Published: 2 February 2011

doi:10.1186/1532-429X-13-S1-O54

Cite this article as: Quick *et al.*: Real-time MR-guided transarterial aortic valve implantation (tavi): in vivo evaluation in swine. *Journal of Cardiovascular Magnetic Resonance* 2011 **13**(Suppl 1):O54.

Submit your next manuscript to BioMed Central and take full advantage of:

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at
www.biomedcentral.com/submit

 **BioMed Central**